

DESCRIPTION

Product	RVP-1450G, Sudan ebolavirus (SUDV) Reporter Virus Particles (RVPs)
Lot	FG-1175B
Strain	Human/Uganda/Gulu/2000
Reporter	GFP
Size	1.0 mL/vial
Packaging	20% FBS/DMEM
Viral Titer	3.47×10^6 TU/mL [†]
Recommended Starting Input	2.5 µL per well (96-well plate) for ≥ 20% infectivity in a flow assay*
Mycoplasma Test	Negative
Manufacture Date	August 2026
Expiration Date	August 2028

SAFETY & HANDLING

Shipping	Shipped on dry ice
Stability and Storage	Store at ≤ -80°C upon receipt

SUDV RVPs are used to test the ability of serum, antibodies, and drugs to neutralize SUDV infectivity. RVPs display antigenically correct glycoprotein pseudotyped on replication-incompetent virus particles that contain a heterologous VSV core. RVPs are capable of a single round of infection and carry a genome that expresses a *Renilla* luciferase reporter gene upon infection. RVPs are produced in HEK-293T cells using plasmids encoding the glycoproteins.

SUDV RVPs are derived from recombinant vesicular stomatitis virus (VSV) from which the VSV glycoprotein gene has been deleted and replaced with a reporter gene (VSVΔG). RVPs are derived from biological materials and should be handled with caution within a BSL2 or enhanced BSL2 laboratory environment. RVPs are not to be used in humans or in animals raised for food.



Thaw tubes in a 37°C water bath for 3 minutes and place on ice until ready to use. RVPs will appear as a translucent, pink solution. Gently mix prior to use and pulse tube for 3 seconds at high speed in a tabletop microfuge to recover all volume from the tube. Vortexing of RVPs should be avoided. Re-freezing of RVPs is not recommended.

[†] Titer is calculated using the estimated number of cells at the end of the experiment, using the following equation:

$$\left[\left(\frac{\% \text{ GFP positive cells}}{100} \right) \times \left(\frac{9,000 \text{ cells}}{1 \text{ well}} \right) \times \left(\frac{1 \text{ well}}{\text{RVP input } (\mu\text{L})} \right) \right] \times \frac{1000 \mu\text{L}}{1 \text{ mL}} = X \frac{\text{Transforming Units (TU)}}{\text{mL}}$$

* Determined using the Vero cell line. Input should be optimized based on specific assay conditions and experimental needs.

INFECTIVITY & NEUTRALIZATION DATA

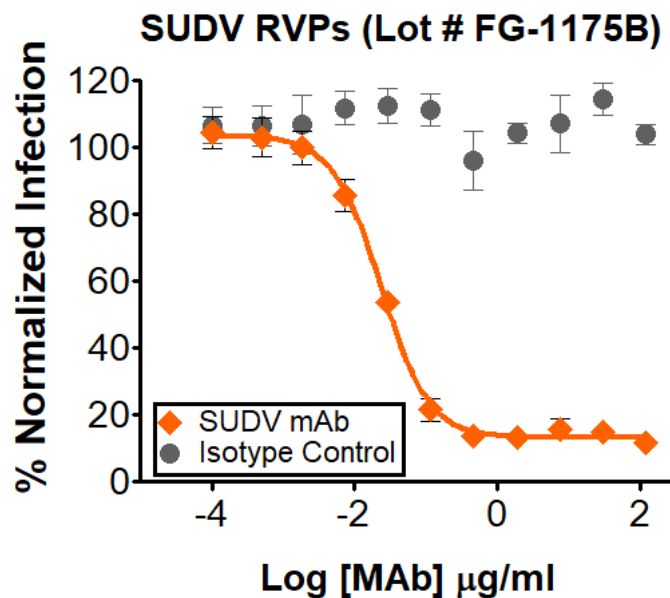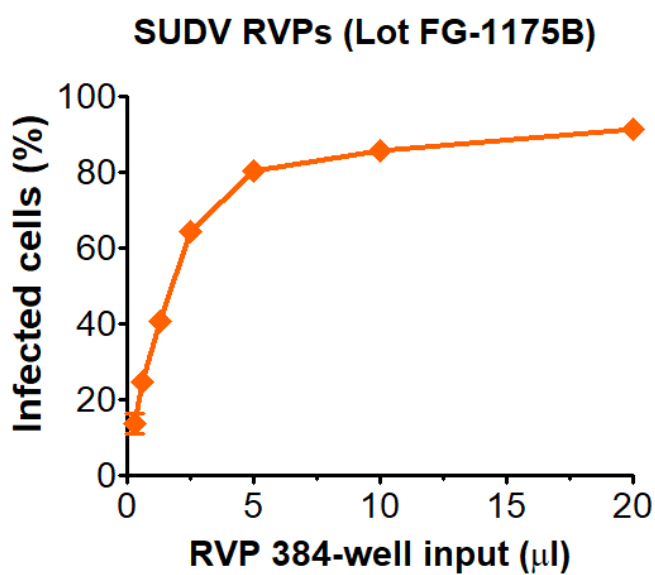

Infectivity and neutralization determined in Vero cells. Infectivity data represent the average $\pm$ SD of technical quadruplicates.

Neutralization utilized 5 μ L of SUDV RVPs in a 384-well plate.

GFP positive cells were detected with an Intellicyt iQue flow cytometer using the BL-1 channel (Ex. 488 nm, Em. 530).

Christina Go, PhD

Senior Application Scientist, Virology

cgo@integralmolecular.com

Integral Molecular

One uCity Square

25 N. 38th Street, Suite 800

Philadelphia, PA 19104

Jennifer Kilgore

Senior Project Manager/Quality Assurance, Virology

jkilgore@integralmolecular.com

Integral Molecular

One uCity Square

25 N. 38th Street, Suite 800

Philadelphia, PA 19104